




The ARC is one of the first N95-equivalent PPE Respirators to be made in Canada. With its superior seal and moisture repellent exterior the ARC provides surgical grade protection when you need it. We have applied our innovative technology and best practices in mask design and manufacturing to create the ultimate in personal protective equipment (PPE) for peace of mind in either healthcare settings or daily life.

# ARC

SURGICAL RESPIRATOR WITH VERTICAL FOLD  
PART NO. 1000-150

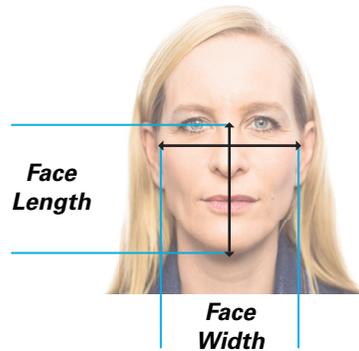

### ARC Respirator: Size Recommendations

Face Length	128.5mm - 138.5mm	R	L	L
	118.5mm - 128.5mm	R	L	L
	108.5mm - 118.5mm	R	R	L
	98.5mm - 108.5mm	R	R	L
		120.5mm - 132.5mm	132.5mm - 144.5mm	144.5mm - 158.5mm
		Face Width		

NOTE: Recommended sizes are not intended to replace proper fit-testing protocols.

### Product Specifications

Product Type	Respirator
Model	ARC
Certification	Health Canada IO No.320544
Style	Vertical Fold
Donning Style	Headbands
Colour	White
Size	Regular / Large
Strap	Polyester / Spandex
Fabric Construction	Polypropylene non-woven
Nose Bridge	Aluminum
Nose Foam	PVC
Packaging	Individually Wrapped
Per Box	25

### Level 3 Protection

Healthcare Applications, Infection Control Practices, Protection from Airborne Pathogens

- Dye free
- Latex free
- Fluid resistant
- Double layer filter
- Comfortable headbands
- Provides protection from small particle aerosols
- Improved face seal prevents leakage around mask

## Performance Results to Industry Standards

Test	Health Canada	NIOSH	Testing Body	Results
Particulate filter efficiency	NIOSH 42 CFR 84 (TEB-APR-STP-0059) ≥95%	NIOSH 42 CFR 84 (TEB-APR-STP-0059) ≥95%	Kinectrics Inc. + NRC	Avg. Filtration Efficiency - 99%
Breathing resistance	42 CFR 84.180 Inhalation < 343.2 Pa Exhalation < 245.2 Pa	42 CFR 84.180 Inhalation < 35 mmH2O Exhalation < 25 mmH2O	Kinectrics Inc. + NRC	Pass Inhalation Resistance - 15.6mm H2O Exhalation Resistance - 13.3mm H2O
Mechanical strength of headstrap	Ability to withstand a 10 N (0.98) kg weight force for each headstrap tested	Not Applicable	PHAC	Pass
Fit (each size)	CAN/CSA Z94.4 Testing done in accordance with NIOSH face panels identified in RCT-APR-STP0005-05a-06, revision 3.0	Not Applicable	Eclipse Innovation Inc.	100% of the subjects passed the fit test with at least one size of mask.
Flammability	16 CFR Part 1610	16 CFR Part 1610	Kinectrics Inc. + Nelson Labs	Pass - Class 1: Burn time ≥3.5s
Fluid Resistance	ASTM F1862 - Standard test method for resistance of surgical mask to penetration by synthetic blood	ASTM F1862 - Standard test method for resistance of surgical mask to penetration by synthetic blood	Kinectrics Inc. + Nelson Labs	Pass - 160 mmHg - ASTM Level 3
Biocompatibility	ISO-10993-1 standard, "Biological Evaluation of Medical Devices Part 1: Evaluation and Testing within a Risk Management Process	ISO-10993-1 standard, "Biological Evaluation of Medical Devices Part 1: Evaluation and Testing within a Risk Management Process	Charles River Laboratories Hungary Kft. + NucroTechnics Inc.	Passed the Cytotoxicity, Skin Sensitization and Dermal Irritation Test

The ARC is the first surgical grade Respirator to be certified by Health Canada for sale in Ontario. It is proudly made in Cambridge, Ontario.

Eclipse Innovations is an Eclipse Automation company. The Innovations group was developed at the start of the COVID-19 crisis, as a direct response to find efficient, reliable solutions given our expertise in the medical device industry.

The Innovations team scoured the globe for best practices in mask automation and manufacturing and then improved upon everything we learned in order to create the ultimate mask products for Canadians, by Canadians.

